## IMPORTANT

- Keep away from direct heat.
- Do NOT attempt to drive or use any other potentially hazardous equipment whilst using the Hand Rejuvenation.
- Do NOT dismantle the control unit, there are no user serviceable parts inside. In the event of a fault, Rio or its service agent or a similarly qualified person must replace it in order to avoid a hazard.
- Do NOT immerse the control unit in water. Wiping with a damp cloth is sufficient to clean the unit.
- Only use the control unit for its intended use.
- This product should only be used and stored at temperatures between 10–50°c and in areas with a humidity level less than 60%.
- Q10 Cream and batteries can be re-ordered by calling our careline on **+44 (0)1242 702345**, using the enclosed re-order form or visiting our website: **www.riobeauty.co.uk**

## WARNING

**The gloves and wrist band contain spandex. Do NOT use if you have a known spandex allergy.**

## CLEANING

**Firstly, ensure the connector leads are removed from the gloves/wrist bands.**

Due to the silver fibres in the gloves, we recommend hand washing only with warm, but not hot water and a little soap. Soak or wash gloves for no more than 5 minutes and allow gloves to dry naturally.

Do NOT use bleach or cleaning agents containing bleach.

## BATTERY INFORMATION

**An intermittent bleep every five seconds with the status light flashing red indicates the battery is low. After 20 seconds the unit will turn itself off.**

TO FIT BATTERY:



Press the clip to open the battery cover. Connect a PP3 9V alkaline battery and replace cover.

If the unit is left unused for a long period of time, remove the battery. Do NOT use rechargeable batteries.

## DISPOSAL

The Waste of Electrical and Electronic Equipment (WEEE) Directive (2002/96/EC) has been put in place to recycle products using best available recovery and recycling techniques to minimise the impact on the environment, treat any hazardous substances and avoid the increasing landfill.

The control unit and batteries are classed as Electrical or Electronic equipment so please ensure that at the end of the life of this control unit and battery, they are disposed of in the correct manner in accordance with local authority requirements. They must NOT be disposed of with household waste.

## CUSTOMER CARE

If you have any questions, or if you experience any difficulties with this product, please call our Rio Careline on **01242 702345**
or email us at: **online@riobeauty.com**

To register your two year guarantee online visit:
**www.riobeauty.co.uk/warranty_online.htm**

| Glove and wrist band material | |
|---|---|
| Silver fibres | 30% |
| Spandex | 5% |
| Nylon | 65% |

CE

Rio® Dezac® and Hand Rejuvenation™ are trademarks of The Dezac Group Ltd
© The Dezac Group Ltd 2011

PO Box 17, Cheltenham Spa, England GL53 7ET
**www.riobeauty.co.uk**

1-IN-GVGL-UK/1.0

# HAND™ REJUVENATION

## PRECAUTIONS

- **Please read all instructions thoroughly and retain for future reference.**
- We do not recommend treatment for people who are pregnant, have a pacemaker, suffer from high or low blood pressure, epilepsy, heart problems, thrombosis, diabetes or skin related illnesses.
- Do NOT repeat treatment within 24 hours.
- Keep out of reach of children and pets. Not for use by or on children under 14 years of age.
- This appliance is not intended for use by persons with reduced physical, sensory or mental capabilities, or lack of experience and knowledge, unless they have been given supervision or instruction concerning use of the appliance by a person responsible for their safety.
- Remove all piercings and jewellery from hands and wrists before use.
- Product contains spandex.

# HAND REJUVENATION

**Hand Rejuvenation uses microcurrent ion technology to pump smoothing and softening agents deep into the skin. The treatment is completed in just 20 minutes.**

## CONTENTS

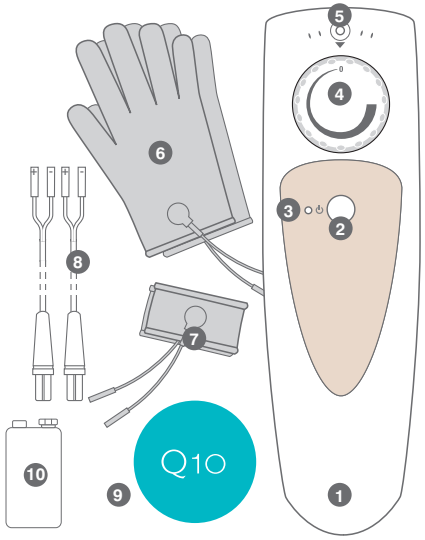


1 Control Unit
2 On/Off Button
3 Status light
4 Output dial
5 Treatment light
6 Gloves with leads
7 Wrist Bands with leads
8 Connector leads
9 Q10 treatment cream
10 PP3 Battery

## PATCH TEST

24 hours before using your Hand Rejuvenation, it is essential to do a patch test. Choose a small area on the inside of your wrist and apply a small amount of Q10 treatment cream. If discomfort or allergic reaction occurs within 24 hours, discontinue use.

## SETUP

The gloves must be connected to the positive (+) socket of the connector lead and the wrist bands to the negative (–) socket to ensure the active ions in the Q10 treatment cream are pumped into the skin.

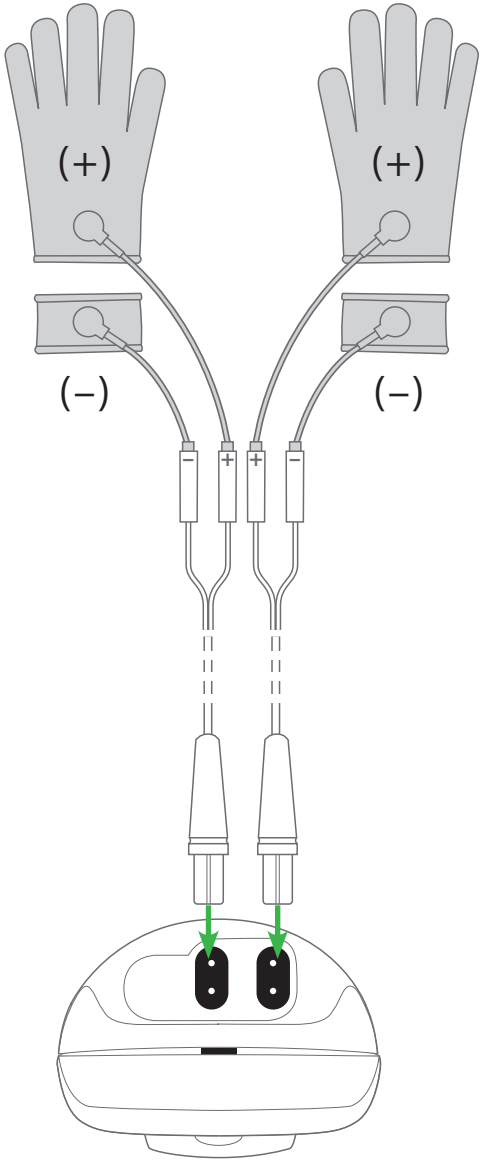


## IMPORTANT

- Ion pump technology uses gentle microcurrents which on higher levels can be felt as a gentle tingling sensation. During treatment, as the active ingredients are pumped into the skin, the tingling sensation will become less noticeable. This occurs over the first 10–15 minutes depending on how much cream is applied.
- For best results initially use daily. Thereafter use as required.
- Always ensure there is a gap between the wrist band and glove.
- Remove all piercings and jewellery from hands and wrists.
- Wash hands and dry before use.

## TREATMENT

**Tip: Start by setting up just one glove to treat one hand. You will then be able to appreciate the difference a single treatment can make.**



**STEP 1**

Plug each glove into the positive (+) socket of the connector lead.



**STEP 2**

Plug each wrist band into the corresponding negative (–) socket of the connector lead.



**STEP 3**

Check the unit is off with the output control set to 0. Plug the two connector leads into the bottom of the control unit.

**Ensure both leads are pushed firmly and fully in.**




**STEP 4**

Apply a generous amount of Q10 cream to the arm where the wrist band will be located. Slip on the elasticated wrist band and position where the cream has been applied.




**STEP 5**

Apply a generous amount of Q10 cream to each hand and put on the glove.

**Ensure there is a gap between the wrist band and glove at all times.**



**STEP 6**

Press the on/off button to switch on. The unit will self test and the status light will illuminate green.

**STEP 7**

Turn the output dial clockwise to start the treatment. Further clockwise movement will increase the intensity. The treatment light will flash to indicate the treatment is in progress. Reduce the intensity by turning the output dial anti-clockwise.

**STEP 8**

The treatment lasts 20 minutes. At the end of the treatment the status light will flash red and the unit will beep for 20 seconds before turning itself off.

**Note The unit can be turned off at any time by pressing and holding the on/off button until the unit beeps 4 times.**